


JMIR

Journal of Magnetic Resonance

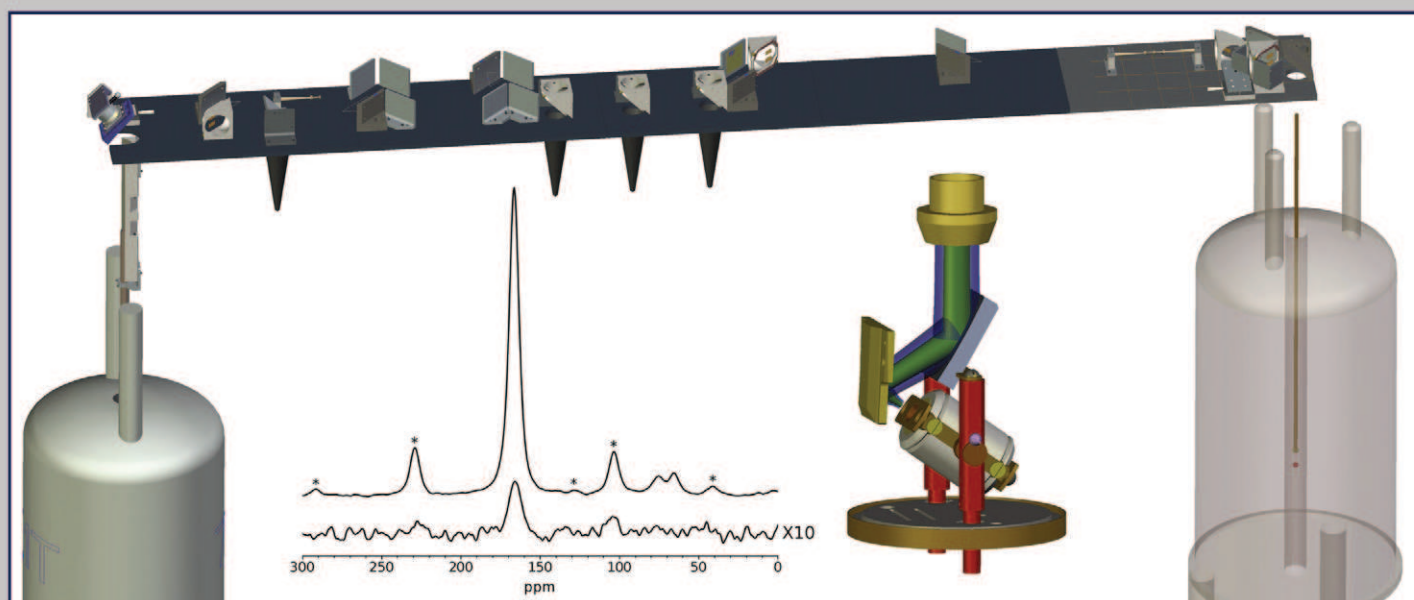

A DNP enhanced MAS NMR spectrometer which uses quasi-optic microwave transmission and a beam focussed into the rotor is described. It gives high-resolution spectra of solids with enhancements of up to x60.

Editor: Lucio Frydman